



Hardware Article

An open-source, programmable pneumatic setup for operation and automated control of single- and multi-layer microfluidic devices



Kara Brower^{a,d,e}, Robert R. Puccinelli^b, Craig J. Markin^c, Tyler C. Shimko^b,
Scott A. Longwell^a, Bianca Cruz^f, Rafael Gomez-Sjoberg^{g,1}, Polly M. Fordyce^{a,b,d,e,g,1,*}

^a Department of Bioengineering, Stanford University, Stanford, CA 94305, United States

^b Department of Genetics, Stanford University, Stanford, CA 94305, United States

^c Department of Biochemistry, Stanford University, Stanford, CA 94305, United States

^d Chem-H Institute, Stanford University, Stanford, CA 94305, United States

^e Stanford Microfluidic Foundry, Stanford University, Stanford, CA 94305, United States

^f Department of Physics and Astronomy, California State Polytechnic University Pomona, Pomona, CA 91768, United States

^g Chan Zuckerberg Biohub, San Francisco, CA 94158, United States

ARTICLE INFO

Keywords:

Microfluidics

Pneumatics

Laboratory automation

Biochip

BioMEMS

Biohacking

Fluid handling

Micro total analysis systems (μTAS)

Quake-style valves

ABSTRACT

Microfluidic technologies have been used across diverse disciplines (e.g. high-throughput biological measurement, fluid physics, laboratory fluid manipulation) but widespread adoption has been limited in part due to the lack of openly disseminated resources that enable non-specialist labs to make and operate their own devices. Here, we report the open-source build of a pneumatic setup capable of operating both single and multilayer (Quake-style) microfluidic devices with programmable scripting automation. This setup can operate both simple and complex devices with 48 device valve control inputs and 18 sample inputs, with modular design for easy expansion, at a fraction of the cost of similar commercial solutions. We present a detailed step-by-step guide to building the pneumatic instrumentation, as well as instructions for custom device operation using our software, Geppetto, through an easy-to-use GUI for live on-chip valve actuation and a scripting system for experiment automation. We show robust valve actuation with near real-time software feedback and demonstrate use of the setup for high-throughput biochemical measurements on-chip. This open-source setup will enable specialists and novices alike to run microfluidic devices easily in their own laboratories.

1. Introduction

Microfluidic technologies enable the precise control and manipulation of fluid at the sub-millimeter scale [1]. Simple, single layer microfluidic devices with channels etched in glass or patterned into soft polymers (e.g. polydimethylsiloxane, or PDMS) have facilitated the study of small-scale fluid phenomena, automated sample loading and common laboratory tasks, and been used for high-throughput compartmentalization of biological reactions [2–9]. More complex multilayer microfluidic devices with monolithic soft polymer valves (also known as Quake-style valves [10,11]) have empowered additional research and commercial applications, including on-chip cell culture and tissue engineering [12], crystallization condition scanning [13–15], single cell analysis [16–18],

DOI of original article: <http://dx.doi.org/10.1016/j.ohx.2017.10.002>

* Corresponding author at: Department of Bioengineering, Stanford University, Stanford, CA 94305, United States.

¹ These authors contributed equally to this work.

E-mail address: pfordyce@stanford.edu (P.M. Fordyce).

<https://doi.org/10.1016/j.ohx.2017.10.001>

Received 11 August 2017; Received in revised form 25 September 2017; Accepted 25 October 2017

2468-0672/ © 2017 The Authors. Published by Elsevier Ltd. This is an open access article under the CC BY-NC-ND license

(<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

high-throughput biochemical analysis [19–21], hydrogel engineering [22–24], and complex fluid handling tasks [11,25].

These multilayer microfluidic devices are typically fabricated in a two-layer geometry, where each layer is made by conventional soft lithography [10]. The ‘flow layer’ contains channels to load and transport samples. The ‘control layer’ contains a series of channels that create and control pneumatically- actuated valves. The two layers are separated by a thin polymer membrane. A valve is formed when flow and control channels of an appropriate size and shape cross [26]. When a control channel is pressurized, the thin membrane deflects into the crossing flow channel to modulate its flow. Both layers require their own set of input lines to interface with on-chip inlets. For complex chips with many control valves, a computer-controlled bank of solenoid valves is typically used to automate control of applied pressure to the valves.

While multilayer devices can serve as powerful tools for a broad range of biological systems [5,27–29], their widespread adoption has been limited, in part, because few detailed open-source protocols and designs for building an automated pneumatic control systems have been published [3,30,31]. Previously, our group worked in conjunction with the Stanford Microfluidic Foundry to publish an open protocol that describes in detail how to fabricate custom multilayer microfluidic devices [32]. In this report, we continue the project of disseminating how-to knowledge on microfluidics by offering designs and detailed step-by-step build instructions for a flexible pressure-driven pneumatic setup that can control both fluid flow and integrated on-chip valves.

The primary pneumatics control system described here allows for automated, programmable control of single and multi-layer microfluidic devices with 48 control lines and 18 individually-addressable flow lines. We present customization options and instructions to build setups from 8 to 96 control lines and 6 to 48 flow lines using this base build. This setup confers several advantages to commercial alternatives including:

- flexible application programming and automation
- remote control to allow experiments to be controlled and monitored outside the lab
- extremely fast valve response times (using Modbus-pulsed solenoid valves)
- very low cost-per-input ratios (both control and flow channel inputs)

The build is modular and easy to customize for a user’s specific needs. We present two modified builds in a later section of the paper for lower complexity control, including a low-cost fully manual control configuration. Previous versions and variants of this setup, originating from the early days of the Stanford Microfluidic Foundry [33], have been used in tens of laboratories resulting in over a hundred peer-reviewed publications ([12,20–23,34,35] are some examples). However, full build details have never been published. Here, we describe the latest optimization of the pneumatic control system in detail to provide a complete tool kit that will allow even labs with little engineering expertise to build all of the instrumentation required for automated microfluidic control.

2. Hardware description

The open-source pneumatic setup and software (Fig. 1) described here can be used for both manual and fully programmable pneumatic control of most PDMS-based microfluidic devices. Our associated software, Geppetto, has both an interactive GUI for manipulating device valves and visualizing their current state (open or closed) as well as command line scripting functionality for automating experiments.

We present 3 build options for the microfluidic pneumatic control system, as listed below. This setup can additionally be expanded for up to 96 control lines and up to 48 flow lines. Control inputs need not correspond to the actual number of valves on the device – only the number of valves needing independent actuation. Typical multilayer microfluidic devices operate with 10–15 control lines and 10–15 sample lines, even for complicated tasks, but this build can accommodate devices with more or fewer inputs or the need to run multiple devices simultaneously on the same setup.

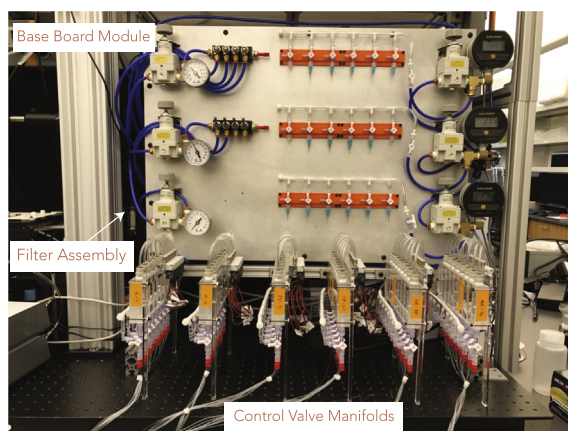


Fig. 1. Photograph of a completed pneumatic build (Option 1) with all 5 build modules.

2.1. Build options

In this paper, we present 3 options for building a microfluidic pneumatic setup:

Option 1: A full build for 18 flow lines and 48 individually addressable solenoid valves to drive 48 control lines for fully automated, programmable and remote operation of complex devices or multiple devices

Option 2: An abridged build for 6 flow lines and 8 individually addressable solenoid valves to drive 8 control lines for fully automated, programmable and remote operation of simpler devices

Option 3: A low-cost build for manual control of 18 flow lines and 12 control lines

The main text will describe the build for **Option 1**. The build is modular and can be easily modified to the simpler builds of **Options 2** and **3** to reduce time and cost, if only limited or manual control of microfluidic devices is needed.

2.2. Module overview

The pneumatics control system is built in 5 **Modules** which are divided by manual and automated control capabilities. **Options 1** and **2** require all 5 **Modules**. The manual build, **Option 3**, requires a modified version of only **Modules 1** and **2**. The builds for **Options 2** and **3** are presented in a **Modifications and Customization Section**.

The Modules are as follows:

- **Module 1:** Base Board, Pressure Regulator Manifolds, and Flow Lines
- **Module 2:** Filter Assembly
- **Module 3:** Control Solenoid Valve Manifolds
- **Module 4:** Control Reservoir Loading Assembly
- **Module 5:** Digital Modbus Control

2.2.1. Manual control modules

This pneumatic setup employs pressure-driven flow control. Microfluidic devices, in general, can be operated either by pressure-driven flow (using constant pressure at the input) or volumetric flow (forcing a set flow rate at the input, as a syringe pump does). Volumetric flow results in unknown pressures inside the flow channels, which makes it difficult to ensure that on-chip valves close reliably and can lead to device delamination. This setup uses pressure-driven flow because it requires little additional equipment beyond common laboratory compressed air sources and provides robust valve actuation on-chip.

Controlling pressure-driven flow rates and actuating on-chip pneumatic valves requires a device-specific pressure range: too little pressure and valves don't close properly, too much pressure and devices can delaminate or become otherwise damaged. Compressed air (from a house air supply, cylinder or compressor) provides a convenient and quiet pressure source but must be adjusted to the correct pressure for microfluidic devices using regulators. **Module 1** (Base Board, Pressure Regulator Manifolds, and Flow Lines) describes the base build for the pneumatic assembly to control input pressures. It contains a base board that mounts regulators for controlling both flow lines and control line manifold pressures as well as fluidic components for sample introduction or manual control of integrated on-chip valves. **Module 2** describes how to connect a filtering assembly to the compressed air source to prevent device contamination and/or clogging of the air regulators.

2.2.2. Automated control modules

Automation of microfluidic valve actuation enables a wide range of additional assays and remote device control but requires additional control hardware. To control on-chip valves, we employ 24 V, three-way, normally open solenoid valves which toggle between an 'open' pressurized state (with pressure from the control manifold regulators in **Module 1**) and a 'closed' atmospheric pressure state to close or open on-chip valves, respectively. These solenoid valves are used to pressurize or depressurize water within a reservoir directly connected to control lines, thereby providing individually-addressable control of each control line. Groups of eight of these solenoid valves are coupled to a plastic manifold containing eight water reservoirs connected to eight chip control lines. We call this assembly a control manifold; these manifolds are built in **Module 3** (Control Solenoid Valve Manifolds). **Module 4** (Control Reservoir Loading Assembly) adds on a large volume water bottle for easy loading and refilling of the water reservoirs in the control manifold. Finally, **Module 5** (Digital Modbus Control) describes the electrical connections between the solenoid valves and a microcontroller (the 'WAGO' fieldbus controller) to allow valves to be digitally controlled by the user via a computer.

2.2.3. Pneumatic control system operation

Combined, these modules constitute all the components and connections necessary to provide pressure-driven flow control and actuate integrated on-chip valves of microfluidic devices. Initial setup of the system for experimental use is described in the **Operation Device Guide**.

While at first glance this setup may seem complicated, we have built multiple setups with researchers of all technical backgrounds with little to no engineering training. Each module is accompanied by a schematic, parts list and illustrated step-by-step build instructions (**Build Guides**) that are included in the [Supplemental Material](#) of this report. The total build takes 1.5 days from start to device testing and is easily managed with 1–2 researchers and common laboratory tools.

Table 1

Cost of hardware for the different build options. See Supplemental Bill of Material for itemized costs.

Build Option	Cost of all associated hardware
#1: Full Programmable Build (48 control lines, 18 flow lines)	\$10,379.65
#2: Abridged Programmable Build (8 control lines, 6 flow lines)	\$4455.14
#3: Manual Build (12 control lines, 18 flow lines)	\$2110.50

2.3. Advantages of an open-source build

Building an open-source pneumatic microfluidic control system has three main advantages to both academic researchers and small companies. First, open source builds are flexible and can be easily modified for a laboratory's needs [30,36]. For instance, this paper describes two easily modified options from the base build in the **Modification and Customization Section**. Second, this build is highly modular; if a component fails or the user prefers a different alternative to a given module (*i.e.*, using an Arduino as opposed to a WAGO PLC), parts can easily be swapped or exchanged. This can be contrasted with commercial closed-source pumps and instruments where exchanges and repairs are often costly and time-consuming. Lastly, the control system described here is significantly cheaper per input than existing solutions, as discussed below.

2.4. Note on associated build costs

This setup has a significantly reduced cost compared to commercial alternatives for the same number of independent input controls. **Table 1** shows the cost of hardware for **Build Option 1** (full build, 48 control lines), **Build Option 2** (modified programmable build, 8 control lines) and **Build Option 3** (fully manual, 12 control lines). The most expensive components are the solenoid valve arrays and WAGO fieldbus digital control modules, which scale directly with the number of independently-addressable control lines needed, as shown in **Table 1**. While the cost of these programmable setups can be significant (\$4455–\$10,380 dependent on number of inputs), commercial solutions cost between \$1500 (lower-end microfluidic syringe pumps, *e.g.* New Era microfluidic syringe pumps ~\$1500, or multi-inlet pressure driven controllers, *i.e.* Fluigent MFCS ~\$1900) to \$5550 (high end pressure-driven pumps, *e.g.* Dolomite P-Pump™) *per independent input*. Consequently, obtaining a similarly programmable pneumatic system for many inputs from commercial suppliers would be > 10X more expensive in the current market than the build described here.

2.5. Hardware summary

- This build describes a pressure-driven pneumatic setup for single- and multi-layer microfluidic device operation. Devices can be operated manually or digitally, enabling remote control.
- The user can customize the number of flow inputs (up to 48) and the number of control inputs (up to 96) for their application.
- The associated software for digital valve control, Geppetto, includes a GUI for fast valve actuation and visualization of current valve states as well as an easy way to script experiments for automated control.
- The build description includes design files to be cut, printed, or machined, as well as overview instructions and step-by-step build guides to construct the setup in 5 different modules, a bill of materials and individual parts list by module, software operation instructions, and an example case for easy construction. These resources can also be found on our Github (https://github.com/FordyceLab/Open_Source_Pneumatics).
- The final setup is ~48" × 24" including the control computer and can be mounted on an optical breadboard, lab bench, or any workspace with either screws or C-clamps.

3. Design files

3.1. Design files summary

The following design files are necessary to complete this build. Downloads of parts in editable file formats (*e.g.* AutoDesk 360 files) are available on the GitHub repository under the Designs folder.

3.2. Description of design files

3.2.1. Build instructions

System_schematic_pneumatics.pdf – Schematic of all parts organized by build module

Bill_of_Materials_pneumatics.xlsx – Multi-sheet parts list, global and by-module (includes modification and custom build Options 2 and 3).

3.2.2. Build and operation step-by-step guides

Module_1_Base_Build_Guide.pdf – Guide for the Module 1 build

Module_2_Filter_Assembly_Guide.pdf – Guide for the Module 2 build
Module_3_Valve_Manifolds_Guide.pdf – Guide for the Module 3 build
Module_4_Control_Loading_Guide.pdf – Guide for the Module 4 build
Module_5_WAGO_Guide.pdf – Guide for the Module 5 build
Operation_Start_Guide.pdf – Instructions for setup initialization and first-time use.
Device_Operation_Guide.pdf – Instructions for device operation and experimental automation.

3.2.3. Laser cut parts

Base Board: *backboard-full* (PDF specifications; DXF for submission to 3rd party) – 28" × 20" backboard to which most components are mounted. Fabrication: ¼" aluminum or acrylic stock. Holes can be drilled or laser cut. Threaded holes hand-tapped as per specifications.

Water Reservoir Stand: *reservoir-stand* (PDF specifications; DXF for submission to 3rd party; STL for 3D printing) – Mounting stand for control manifold water reservoirs. Fabrication: ¼" aluminum or acrylic stock. Threaded holes hand-tapped as per specifications. Alternatively, can be ordered from local plastic suppliers/3rd party, or 3D printed on printers with a sufficiently large workspace.

3.2.4. Optional modified laser cut parts

3.2.4.1. Base board alternatives. *backboard-left* (PDF specifications; DXF for submission to 3rd party) – The left 10.5" of *backboard-full*. Its reduced size enables fabrication on laser cutters with smaller workspaces. It should be used with *backboard-right*; if this component is used, *backboard-full* is not needed. ***backboard-right*** (PDF specifications; DXF for submission to 3rd party) – The right 17.5" of *backboard-full*. Same specifications as above. ***backboard-left-lc*** (PDF for laser cutter) – Variation of *backboard-left* specifically for direct conversion to a Universal Laser Systems file format (lines are 0.02 mm wide, [255,0,0] RGB). Please verify that the file format is compatible with your laser cutter. ***backboard-right-lc*** (PDF for laser cutter) – Variation of *backboard-right* specifically for direct conversion to a Universal Laser Systems file format (lines are 0.02 mm wide, [255,0,0] RGB). ***reservoir-stand-lc*** (PDF for laser cutter) – Variation of *reservoir-stand* specifically for direct conversion to a Universal Laser Systems file format (lines are 0.02 mm wide, [255,0,0] RGB).

3.2.5. Machined parts

Control Water Reservoirs: *reservoir* (PDF specifications; DXF for submission to 3rd party) – Control manifold reservoirs used to hold water for control lines. Fabrication: 1" acrylic stock. Custom machined in-house or by 3rd party.

3.2.6. 3D printed parts

Flow Control Manifold: *stopcock-mount* (STL for printing) – Mount for 3 stopcocks that control flow line pressurization. Fabrication: ABS plastic or similar.

3.2.7. Open-source software

Geppetto (Github Repository) – Python pneumatic control software with Kivy GUI and optional Windows binary. A Read Me file and all code dependencies are included in the repository unless noted. Example files are included in the repository.

Geppetto CLI (Github Repository) – Python pneumatic control software for command line scripting (command line integration, CLI) to automate experiments. A Read Me file and all code dependencies are included in the repository. Example files are included in the repository.

4. Bill of materials

4.1. Master bill of materials

The following is a global list of materials to be purchased before the build. Material quantities should be adjusted to the needs of your build. The main build (**Build Option 1**) used as an example in the following Build Guides is for 18 flow line inputs and 48 individually-addressable control line inputs. Materials lists for modified **Build Options 2** and **3** are presented in the **Modification and Customization Section**.

A more detailed Bill of Materials with purchasing links and further information is available as [Supplement 2](#) and is updated often on our Github repository and available on our OSF registration.

5. Build instructions

5.1. Overview of multi-component build

This build takes place in 5 discrete modules that eventually interconnect. The following general build schematic describes all the parts and connections necessary to complete the build ([Fig. 2](#)). For each module, we describe the module operation and provide a ‘close up’ version of the schematic compared to the final implementation of that assembly. Assembly details are presented step-by-step in detail in a series of 5 build guides in the [Supplemental Information](#) of this article. The end result will be a pressure-driven

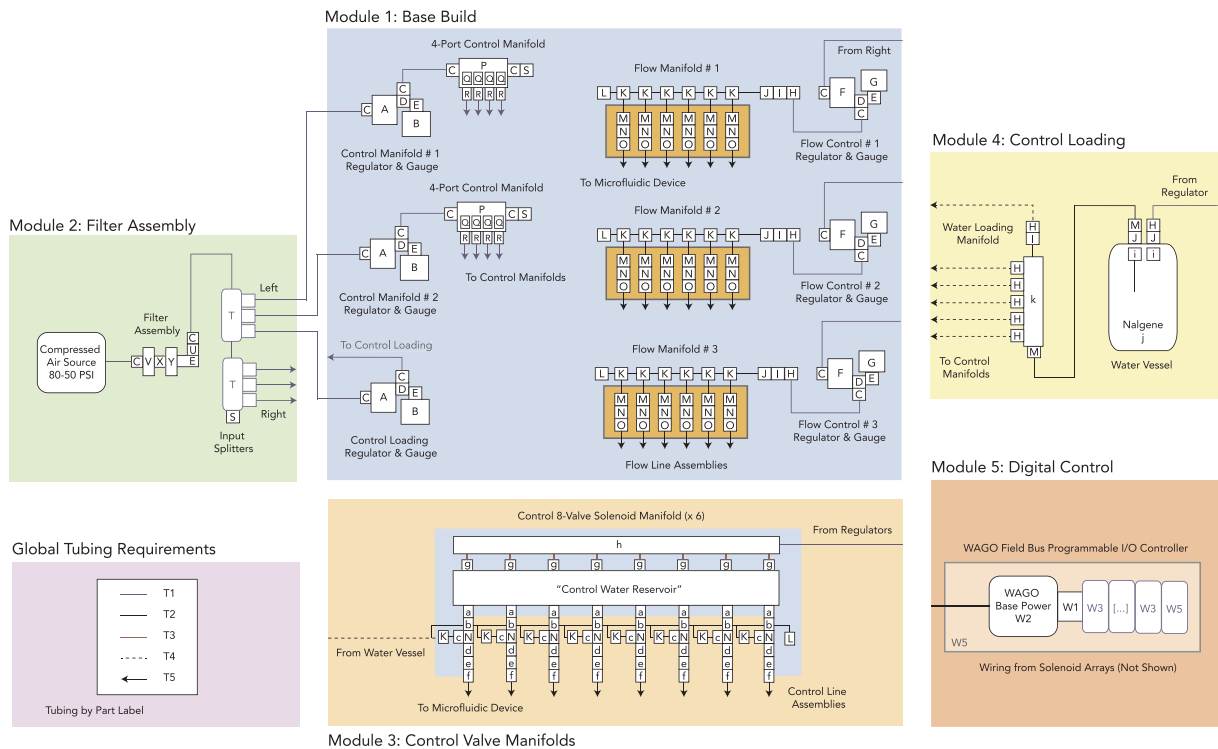


Fig. 2. Overall setup schematic with parts designated by letter and number (as referenced to the Bill of Materials).

pneumatic setup for automated device control that is ready to use.

The following sections describe the details for the main **Build Option 1**. These sections can be used as examples for **Build Options 2** and **3** but will need to be adjusted accordingly to the schematics presented for those options, as shown at the end of this paper.

5.2. Module 1: base board, pressure regulator manifolds, and flow lines

This module describes the main base build for the setup (Fig. 3). Each build has air regulators to control the pressures used to drive manual flow and valve lines. As different on-chip flow inputs may require different pressures, the board contains several different ‘flow’ regulators to control pressures to the flow line manifolds mounted on the base board (right side regulators). In the main build, 3 regulators control 18 flow lines as shown in Fig. 2. Digital gauges provide highly precise low-range (0–20 psi) flow control and are powered by the WAGO modus controller described in **Module 5**. The manual build, **Build Option 3**, replaces these digital gauges with low-range (0–10 psi) analog gauges for a cost-effective alternative, with some sacrifice to measurement precision.

For automated builds (**Builds 1** and **2**), regulators also supply pressure for the banks of control solenoid valve manifolds that ultimately pressurize the control lines and actuate on-chip microfluidic valves (left side upper regulators). In the main build, 2 regulators control pressurization of the control solenoid manifolds and modulate their pressurization via mounted switchboxes (left side). These switchboxes connect directly to the 8-valve manifolds presented in **Module 3**. The regulators used here can be relatively imprecise as long as they provide pressure regulation in the range needed to close microfluidic devices (0–60 psi). Manual versions are sufficient. Automated builds further have an integrated option to load and refresh the control manifold valve banks with water easily. In the main build, a regulator (left side bottom regulator) is dedicated to this task and connected to the control loading assembly in **Module 4**. These components are mounted to a single base plate for convenient adjustment and connection between modules. The build guide provides instructions on how to mechanically connect all components to the base plate and pneumatically connect components to one another.

To build this module, follow the [Module_1_Base_Build_Guide.pdf](#) (Supplement 3).

5.3. Module 2: filter assembly

This module inserts a filter assembly between the compressed air source and the regulators on the Base Board (**Module 1**) to keep oil or small particulates in the pressurized air from contaminating the regulators and on-chip valves in critical experiments (e.g. long-term cell culture or on-chip enzymatic assays) (Fig. 4). This assembly can be replaced by cheaper disposable filters if desired.

To build this module, follow the [Module_2_Filter_Assembly_Guide.pdf](#) (Supplement 4).

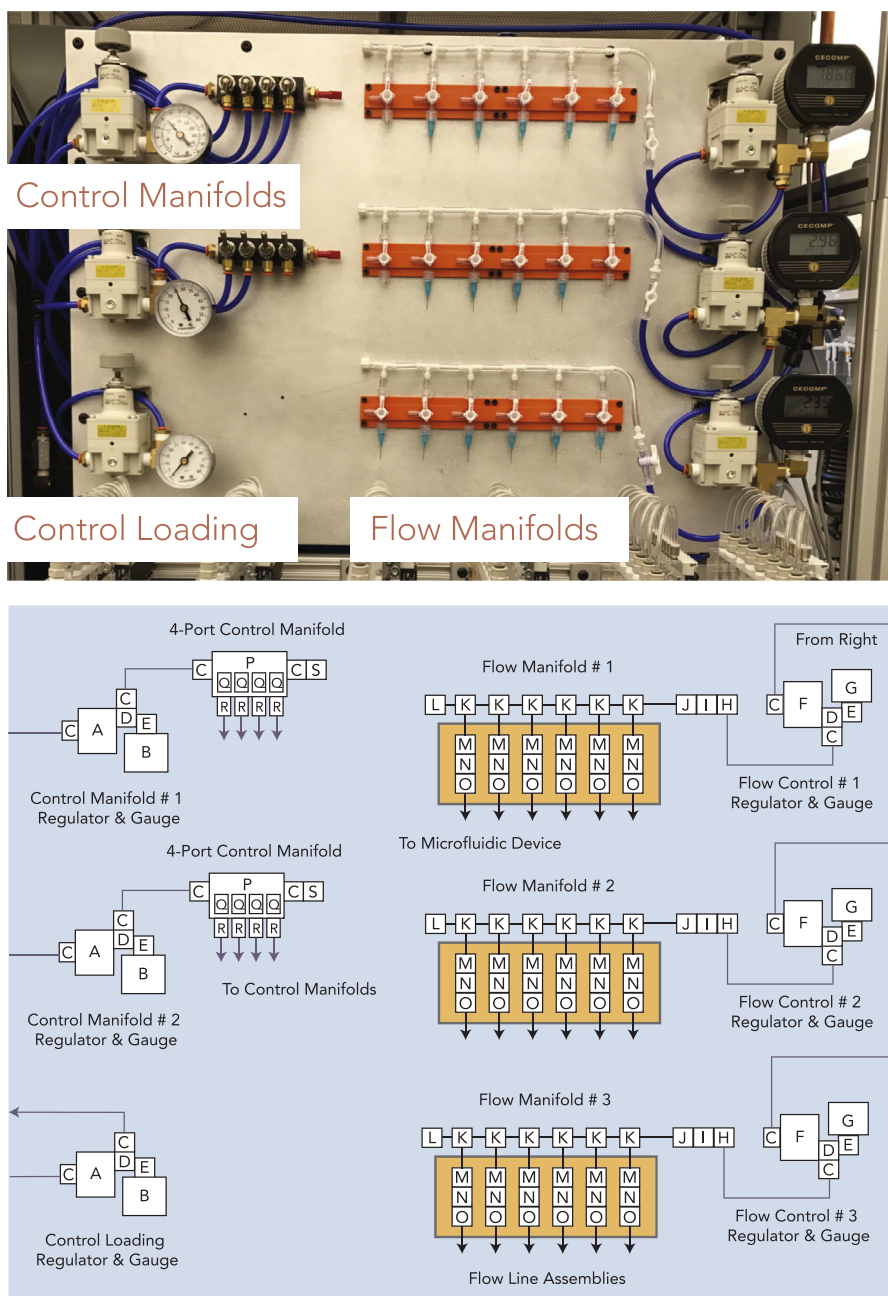


Fig. 3. (a) Module 1 schematic. (b) Finalized implementation of Module 1.

5.4. Module 3: control 8-valve solenoid manifolds

This module creates the hardware necessary for automated valve actuation. The main build has 6 sets of Control Valve Manifolds that actuate on-chip valves by pressurizing water-filled Tygon control lines connected to on-chip control channels (Fig. 5). Each Control Valve Manifold has 8 water reservoirs connected to 8 solenoid valves with independent actuation. Each solenoid valve is individually driven by a 24 V signal supplied by the fieldbus controller of Module 5. When actuated, each solenoid pressurizes a water reservoir (pressure sent from the Base Board – Module 1) and its connected control line input to the microfluidic device to close dead-end valves. The water reservoirs also have a loading function (via a separate fluidic circuit activated by toggling the manifold stopcocks) so that water can be refreshed via Module 4.

Fast valve pressurization is often critical for many microfluidic assays including on-chip biochemical assays, droplet generation, microfluidic sorting and precise fluidic dosing using on-chip pumps [20,22–24,35]. The Festo 24 V solenoid valves used here, while expensive, offer superior response times essential for fast valve actuation as well as reliable state switching with long lifetime

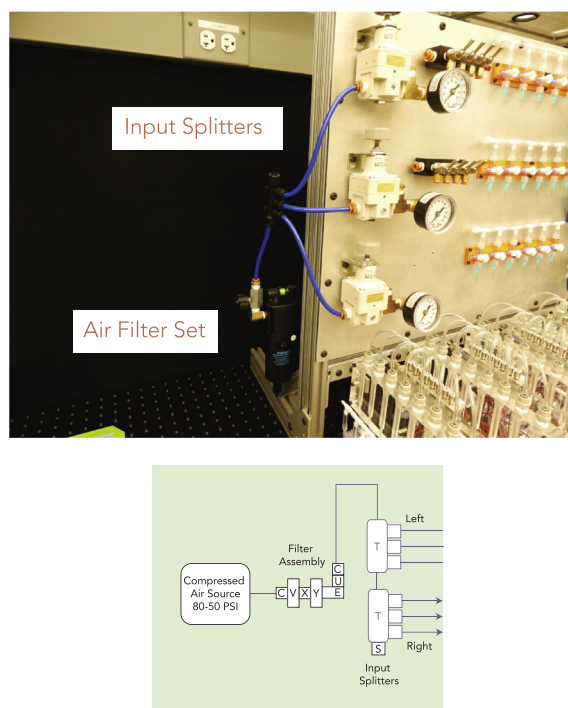


Fig. 4. (a) Module 2 schematic. (b) Finalized implementation of Module 2.

(> 5 years operation). The response times of these solenoid valves is ~ 4 ms response from pulse. Full fluidic valve actuation on-chip from the digital pulse is on the order of 7–20 ms, dependent on valve and device geometry. The three-way, normally-open solenoid valves in this setup toggle between atmospheric pressure and compressed air as set by the regulators of **Module 1**, allowing lines to be vented to atmosphere when not in use (two-way valves lack the ability to vent lines or depressurize lines to open valves). The use of normally-open solenoid valves allows on-chip valves to return to a safe ‘closed’ position in the event of an unexpected software crash or power interruption. In addition, these valves are additional very low profile, easily allowing parallelization as demonstrated in this build.

To customize the build, control lines can be filled with oil or buffer instead of water to reduce osmotic water transfer between control and flow lines. Three-way solenoid valve arrays can also be connected to other air sources to toggle between different states (e.g. vacuum and compressed air, vacuum and atmospheric pressure – instead of atmospheric pressure and compressed air), if needed.

To build this module, follow the [Module_3_Valve_Manifolds_Guide.pdf](#) (Supplement 5).

5.5. Module 4: control reservoir loading assembly

Maintaining water in the water reservoirs is essential for properly pressurizing control lines as air within the lines can create uneven closing times across the devices and nucleate bubbles in the flow channel in long-term experiments. This module builds a pressure vessel and associated tubing for loading water into the water reservoirs of the Control Valve Manifolds from **Module 3** to prevent control line drying (Fig. 6). While loading the water reservoirs can be completed without this pressure vessel assembly (e.g. using tubing), this assembly simplifies the water loading process. Water is loaded by pressurizing the water vessel (driven from a regulator in **Module 1**) and switching the relevant manifold stopcock so that water flows into the manifold. Further details can be found in the [Device Operation Guide](#).

To build this module, follow the [Module_4_Control>Loading_Guide.pdf](#) (Supplement 6).

5.6. Module 5: digital modbus control

This module adds computer-based control of valve actuation (Fig. 7). A WAGO programmable logic controller (“Fieldbus controller”) is used to send 24 V pulses to actuate the solenoid valves of **Module 3** individually, as well as power the digital gauges of **Module 1** (note: these gauges can be powered without the WAGO, but the WAGO provides a convenient integration of all electronic components in this context). The WAGO controller accepts a wide variety of input/output modules (“brick modules”) to create flexible and scalable control systems. The build presented here includes a power supply module for global power and ground, the WAGO controller CPU module with Ethernet connectivity, a series of 24 V digital output (DO) modules for controlling valve states, and a 5 V output module for powering auxiliary devices (e.g. digital gauges or hardware requiring TTL inputs). A computer can communicate with the WAGO fieldbus controller over Ethernet using a standard protocol called MODBUS. These communications are

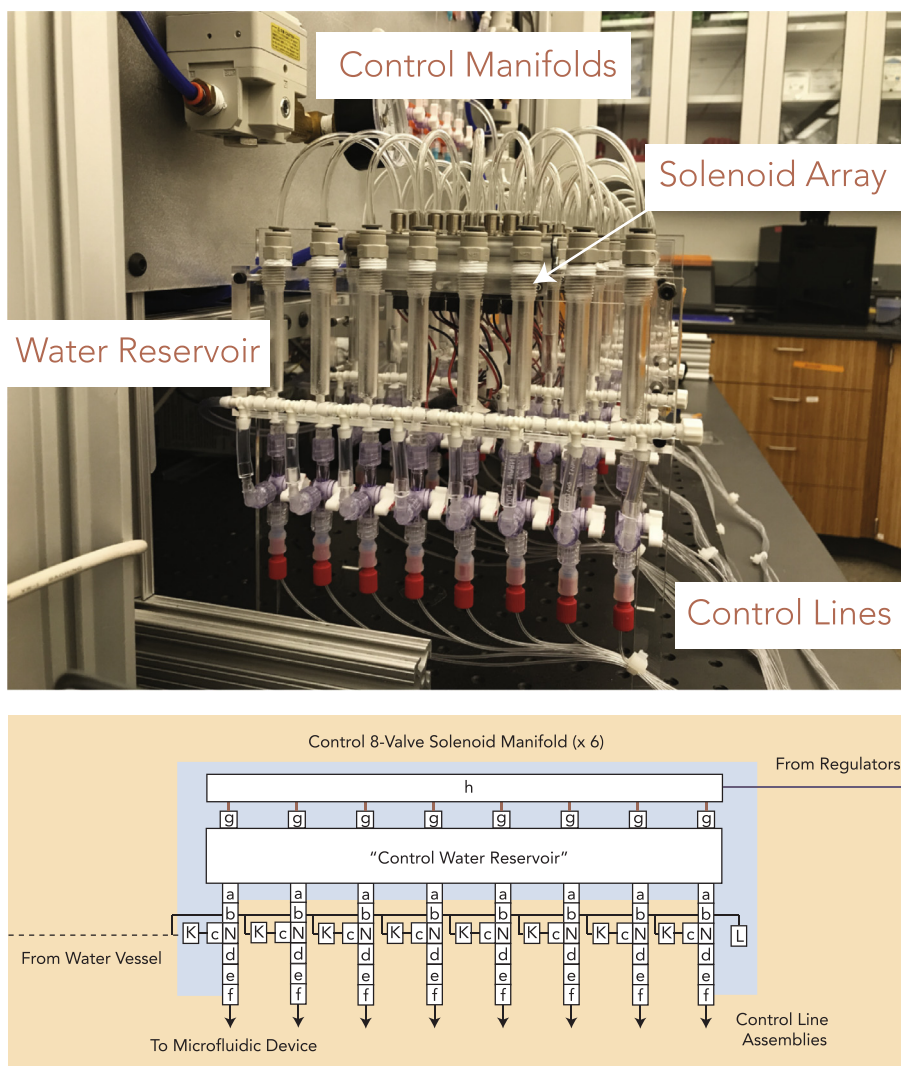


Fig. 5. (a) Module 3 schematic. (b) Finalized implementation of Module 3.

abstracted from the user using our Geppetto GUI or CLI software. Full wiring and computer setup details are reviewed in the Build Guide for this module.

For project-specific customization, it should be noted that the 4-way DO modules we have chosen send out digital signals that switch between 0 V (float) and 24 V (high-side control). Modules for more complex tasks such as digital in (DI) or mixed DO/DI modules can be swapped in or out depending on your needs (e.g., for additional equipment control). Alternatives to the WAGO controller (such as a USB controller [33] or Arduino PLCs, presented by White and colleagues in this issue) can be used but current and voltage compatibilities with the Festo solenoids should be checked before wiring.

To build this module, follow the [Module_5_WAGO_Guide.pdf](#) (Supplement 7).

6. Modification and customization

The pneumatic setup outlined here can easily be customized for your laboratory's needs. Each component is highly modular, enabling easy part exchanges. Our Build Guides contain useful advice on our own trials using different part alternatives, when applicable. To demonstrate the ability to modify the base build, we present two additional build options with accompanying schematics. To build these options, simply use the previous Build Guides as needed for each part; component installation is exactly the same. The fully manual build, **Build Option 3**, does not use **Modules 3, 4, or 5**.

Option 2: An abridged build for 6 flow lines and 8 individually addressable solenoid valves to control 8 control lines that fully automated, programmed and remotely operated for simpler devices

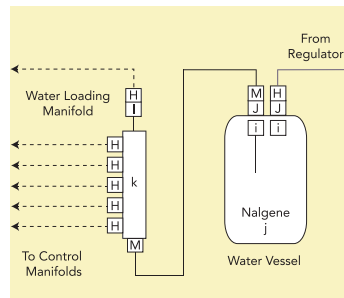
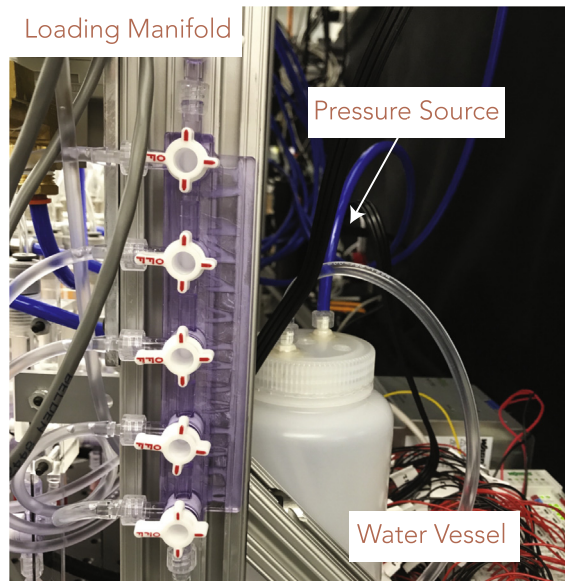


Fig. 6. (a) Module 4 schematic. (b) Finalized implementation of Module 4.


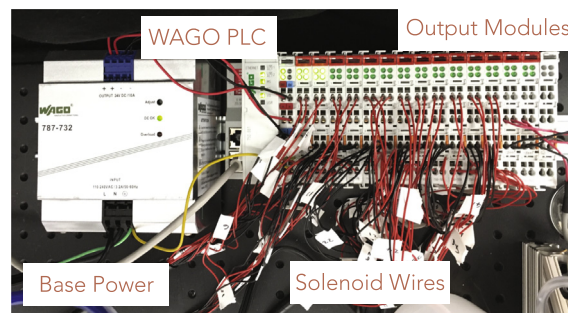


Fig. 7. (a) Module 5 schematic. (b) Finalized implementation of Module 7.

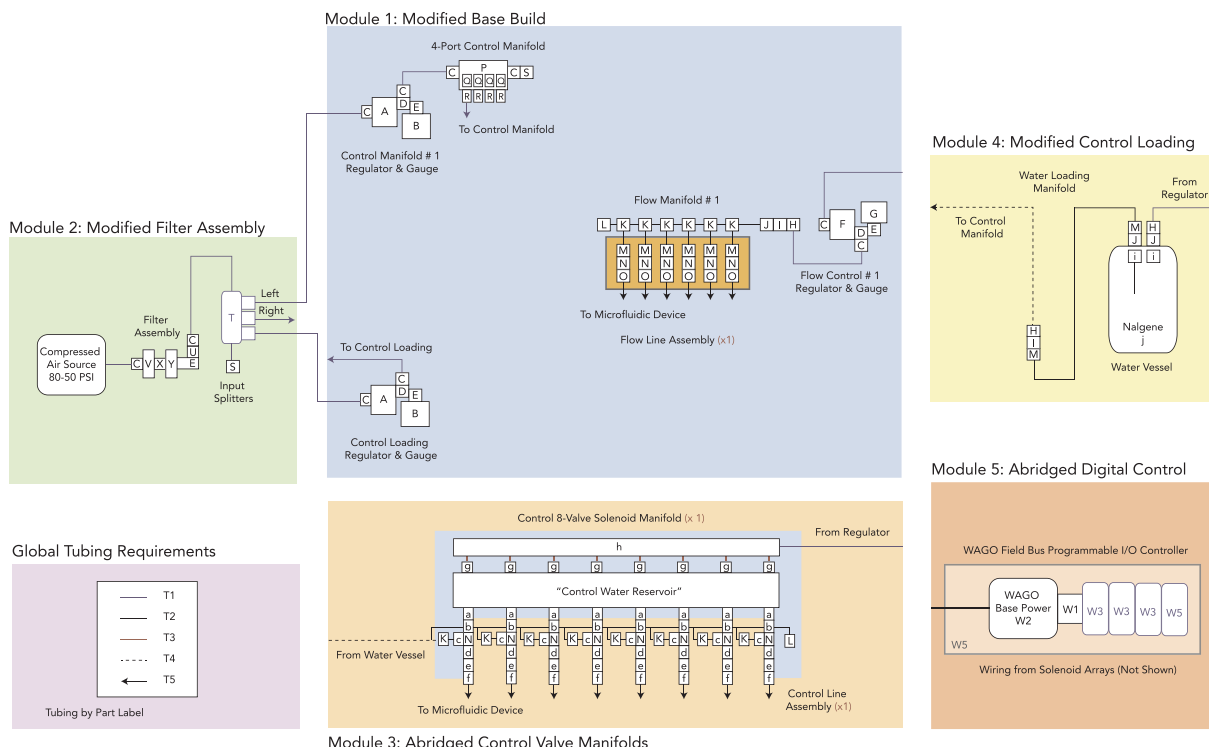


Fig. 8. Build Option 2 schematic.

To build this option, follow the **Option 2 Build Materials List** (Supplement 2, Bill of Materials Sheet 2) (Fig. 8).

Option 3: A fully manual build for 18 flow lines and 12 manually addressable control lines without automation capabilities which can be used to save costs (Fig. 9)

To build this option, follow the **Option 3 Build Materials List** (Supplement 2, Bill of Materials Sheet 3).

7. Operation instructions

After completing the build, it is now time to begin the exciting process of testing and operating the first microfluidic device with your new setup! Before beginning, follow the initialization guide **Operation_Start_Guide.pdf** (Supplement 8) to pressurize and check for leaks in the system.

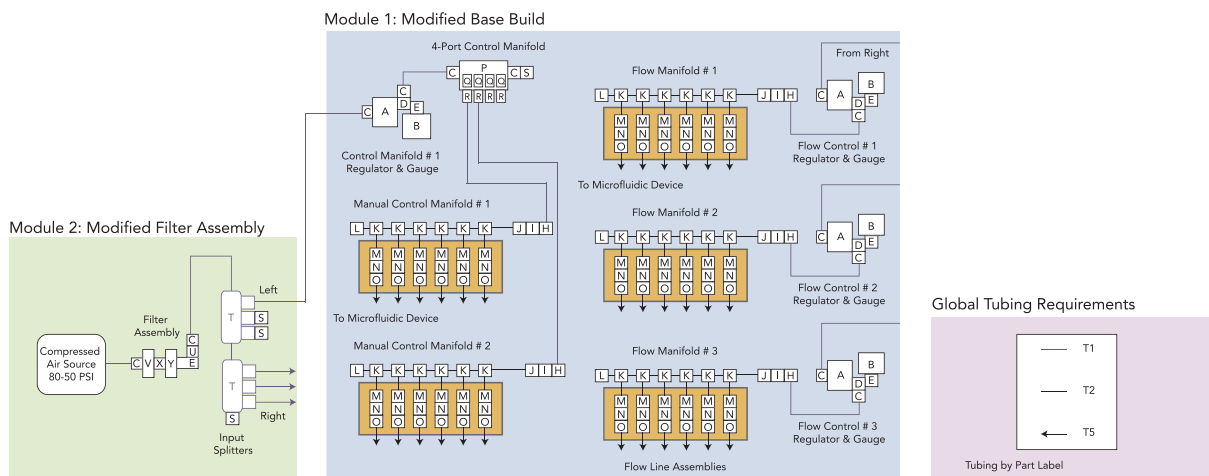


Fig. 9. Build Option 3 schematic.

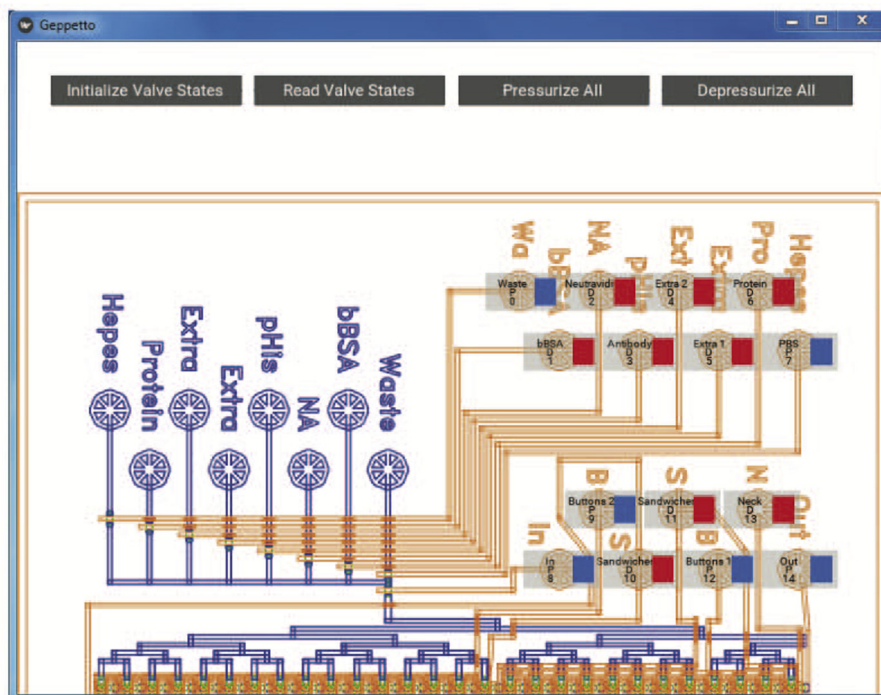


Fig. 10. Example Geppetto GUI for valve state visualization of a microfluidic device. Shown here is the custom GUI configured for the MITOMI demo device (see Section 9).

7.1. Geppetto: python operation and scripting

We recommend operating your microfluidic device using our pneumatic control software, which enables valve state visualization and control as well as scripting. Alternatively, users can write their own MODBUS implementation for talking to the WAGO, if desired. Geppetto is a Python-based pneumatic control software built using the Kivy graphical user interface framework for GUI development. Geppetto's GUI supports nearly any user-defined control layout, with the ability to change the background image and the placement of the control buttons to match any user-designed device using a simple YAML config file.

To customize Geppetto for your own microfluidic device, use the Read Me under our Github release available at <https://github.com/FordyceLab/geppetto>. If you are unfamiliar with Python, an excellent tutorial can be found here (<https://docs.python.org/3/tutorial/index.html>) on how to install and operate Python on your machine.

If your lab feels more comfortable using MATLAB, we have also set up a fully scriptable MATLAB valve control system available at https://github.com/FordyceLab/PneumaticControl_MATLAB that we used in a Jove video protocol of device operation we published recently [32], though we recommend the use of Geppetto because of its improved ease-of-use.

After installing Geppetto, load an image of the device design according to instructions in the Read Me and adjust valve locations to the correct positions in the image. The final image should look similar to the following (Fig. 10).

7.2. Operating a chip

To operate a microfluidic device, follow the steps **Device_Operation_Guide.pdf** (Supplement 9).

To summarize:

1. Connect the control lines and flow lines to the device.
2. Pressurize the control and flow regulators to the desired pressures and toggle the control manifold switches to send pressure into the control manifolds.
3. Use Geppetto to actuate the valve states.

We previously published a Jove video protocol of a device run that may be useful for visualization of this process [32].

7.3. Automating microfluidic experiments

Geppetto also allows scripting of valve actuation events and wait times to automate microfluidic experiments. Scripting occurs in

Table 2
Design file summary.

Design file name	File type	Open source license	Location of the file
System Schematic	PDF	GPL	Available with the article
Bill of Materials, Detailed with Links	XLSX	GPL	Available with the article
Build Guides	PDF (multiple)	GPL	Available with the article
Base Board (<i>backboard-full</i>)	PDF DXF	GPL	OSF: https://osf.io/jwyau Github: github.com/FordyceLab/Open_Source_Pneumatics
Flow Control Manifolds (<i>stopcock-mount</i>)	STL	GPL	OSF: https://osf.io/jwyau Github: github.com/FordyceLab/Open_Source_Pneumatics
Water Reservoir Stand (<i>reservoir-stand</i>)	PDF DXF STL	GPL	OSF: https://osf.io/jwyau Github: github.com/FordyceLab/Open_Source_Pneumatics
Control Water Reservoir (<i>reservoir</i>)	PDF DXF	GPL	OSF: https://osf.io/jwyau Github: github.com/FordyceLab/Open_Source_Pneumatics
Geppetto Geppetto CLI	Python code	GPL	OSF: https://osf.io/jwyau Github: https://github.com/FordyceLab/geppetto Github: https://github.com/FordyceLab/geppetto-cli

the command line using the Geppetto CLI program (<https://github.com/FordyceLab/geppetto-cli>). Use the Read Me to set up your first scripting experiment. Example files (e.g. the script for our example experiment below) can be found under the Scripts folder (See [Tables 2–4](#)).

8. Validation and characterization

The pneumatics control setup described here has been used in our laboratory for multiple studies, including the microfluidic generation of hydrogel microparticles [32], microfluidic synthesis of lanthanide-encoded beads [24], and high-throughput biochemical affinity measurements on-chip [35]. Here, we describe an example microfluidic experiment using the full pneumatic build, Geppetto CLI, and a microfluidic device, MITOMI (as described previously [19,20,35]) for high-throughput affinity measurements.

8.1. Confirmation of multi-valve pressurization and state change

[Fig. 11](#) shows a brightfield image of multiple valve opening and closing events on chip, with valve state controlled via the Geppetto GUI. [Supplement 10](#) is a video of valve toggling events, demonstrating individually-addressable valve control (See [Fig. 12](#)).

8.2. Characterization of valve closing pressures and response times for multiple device geometries

We have characterized required microfluidic valve control pressures across a wide range of device geometries. “Push-down” devices (control layer on top) fabricated via standard soft lithography techniques tend to operate at 15–20 psi for complete valve closure. “Push-up” devices (control layer on bottom) can tolerate higher pressures (e.g. these devices are more resistant to delamination) and operate from 10 to 40 psi (or higher). For a given channel geometry, push-down valves require higher pressures to close than push-up valves [2,10,11]. The appropriate valve closing pressures can be determined by the user for new device geometries by introducing beads or food dye into the flow channel, varying input pressures, and visualizing whether all the fluid is completely excluded beneath the valve.

8.3. Automating a microfluidic experiment

To demonstrate the automation potential of the setup, we scripted an experiment in Geppetto to carry out successful surface patterning of a MITOMI device. MITOMI is a microfluidic device that has been employed for many high-throughput biochemical measurements, most notably for assessing thousands of transcription factor (TF) binding affinities to DNA sequences printed on a glass slide [19,20,35]. MITOMI devices contain hundreds to thousands of individual pairs of chambers with multiple types of valves (e.g. a neck valve for connecting chamber pairs, button valves for patterning specific areas in a larger chamber, and sandwich valves for isolating chambers from one another) for performing biochemical affinity measurements.

In our experiment, we performed a simple multi-step surface functionalization to pattern anti-eGFP in a small circular area in each chamber pair using the ‘button’ valves of the device, which protect the glass surface from interacting with introduced solutions when activated. We automated the experiment using scripting in Geppetto CLI. Our script ([Supplement 11](#)) outlines the valve actuation events and flow times. Further details on this experiment program can be found at <https://github.com/FordyceLab/MITOMI-geppetto>.

In particular, we created a patterned circle of anti-eGFP antibodies on the glass slide surface in the “push-down” device via the following steps: (1) open button valve, (2) introduce biotinylated BSA, (3) wash, (4) introduce neutravidin, (5) wash, (6) close button,

Table 3

Full Build (Build Option 1) Bill of Materials by Module. Parts are purchased by Module. Any “0” quantity denotes that a multi-part pack has been previously purchased of sufficient size to provide all additional parts needed for the Module in question. Links to manufacturer sites are included in the Bill_of_Materials_pneumatics.xlsx supplemental file (Supplement 2).

Global requirements by module for full build						
Table 1: Global Tubing Requirements						
Component	Source	Catalog Number	Quantity	Cost /Unit	Total	Part
1/4" OD × 1/8" ID polyurethane tubing, blue, 50 ft roll	McMaster-Carr	5648K74	1	\$29.00	\$29.00	T1
1/4" OD × 1/8" ID Tygon tubing, clear, 50 ft roll	McMaster-Carr	6516T14	1	\$40.50	\$40.50	T2
5/32" OD × 3/32" ID polyurethane tubing, clear, 100 ft roll	Pneumadyne	PU-156F-0	1	\$17.00	\$17.00	T3
3/16" OD × 1/8" ID Tygon tubing, opaque, 50 ft roll	Grainger	2LPR9	1	\$17.41	\$17.41	T4
Tygon ND-100-80 Tubing (500' roll, 0.06" OD, 0.02" ID)	Fisher Scientific	14–171-284	1	\$317.00	\$317.00	T5
Spirally-Cut Cable Wrap, 3/8" O.D., Black Polyethylene	M.M. Newman Corp.	HT 3/8 UR-25	1	\$14.98	\$14.98	T6
Table 2: Pneumatic Control System, Module I: Base Board, Pressure Regulator Manifolds, and Flow Lines						
Component	Source	Catalog Number	Quantity	Cost /Unit	Total	Part
Double Standard Solid 80/20 Rails (26" × 2" × 1")	McMaster-Carr	47065T803	2	\$21.06	\$42.12	b1
Single Standard Solid 80/20 Rails (26" × 1" × 1")	McMaster-Carr	47065T848	3	\$9.36	\$28.08	b2
Double Standard Hollow 80/20 Rails (12" × 2" × 1")	McMaster-Carr	47065T107	2	\$9.13	\$18.26	b3
Diagonal 80/20 Rail (6" × 1" × 1")	McMaster-Carr	47065T186	2	\$15.67	\$31.34	b4
Standard End Feed Fasteners, Pack of 4	McMaster-Carr	47065T142	6	\$2.30	\$13.80	b5
Elbow Bracket 4-Hole Extended Corner Bracket	McMaster-Carr	47065T239	8	\$5.85	\$46.80	b6
Extended Corner 8-Hole Fastener	McMaster-Carr	47065T253	2	\$8.79	\$17.58	b7
Corner 5-Hole Surface Bracket	McMaster-Carr	47065T267	2	\$8.47	\$16.94	b8
10-32 1/2" Socket Head Screws, Pack of 100	McMaster-Carr	91251A342	1	\$9.60	\$9.60	s1
6/32 1-1/2" Partially-Threaded Socket Head Screws, Pack of 50	McMaster-Carr	91251A157	1	\$9.94	\$9.94	s2
6-32 1/4" Socket Head Screws, Pack of 100	McMaster-Carr	91251A144	1	\$8.46	\$8.46	s3
SMC Precision Air Regulator, 1/4" ports, 60 psi upper range	Stevens Engineering	IR2010-N02	3	\$75.80	\$227.40	A
Pressure Gauge, 1/4" Back Connector, 0–60 psi	McMaster-Carr	4000K791	3	\$12.03	\$36.09	B
1/4" NPT to 1/4" Brass Push-to-Connect Tube Fitting	McMaster-Carr	7880T125	16	\$2.24	\$35.84	C
Brass Tee Fitting, 1/4" NPT, FxFxM	McMaster-Carr	50785K222	6	\$4.90	\$29.40	D
Brass Elbow Fitting, 1/4" NPT, FxM	McMaster-Carr	50785K43	6	\$2.50	\$15.00	E
Precision Air Regulator, 1/4" ports, 30 psi lower range	Stevens Engineering	IR2000-O2-A	3	\$75.80	\$227.40	F
Digital Pressure Gauge, 1/4" MNPT, 0–30 psi	McMaster-Carr	3943K15	3	\$428.45	\$1285.35	G
Male Luer Integral Lock Ring, 400 series, 1/8" barb, Pack of 100	Value Plastics	MTLL430-9002	1	\$20.20	\$20.20	H
1-Way Luer Stopcock, M Lock, Pack of 100	Cole-Parmer	Sk-30600-05	1	\$185.00	\$185.00	I
Female Luer 1/4"-28 Panel Mount to 1/8" Barb, Pack of 100	Value Plastics	FTLLB230-1	1	\$19.00	\$19.00	J
Tee Tube Fitting for 1/8" ID Tubing, Pack of 100	Value Plastics	T230-1	1	\$26.80	\$26.80	K
Luer Plug Caps, Pack of 10	McMaster-Carr	51525K311	1	\$2.41	\$2.41	L
Male Luer Integral Lock Ring, 1/8" barb, Pack of 100	Value Plastics	MTLL230-9	1	\$20.20	\$20.20	M
4-Way Luer Stopcock, M Lock, F Connectors, Pack of 100	Cole-Parmer	EW-30600-09	1	\$185.00	\$185.00	N
Blunt Stainless Steel Luer Lock Needle, Pack of 50	McMaster-Carr	75165A684	1	\$11.88	\$11.88	O
4-Station Control Manifold, 1/4" NPT-F inlets, 1/8" NPT outlets	Pneumadyne	M10-125-4	2	\$12.60	\$25.20	P
Dented Toggle Control Switch, 1/8" NPT input, 10/32" output	Pneumadyne	C030621	8	\$14.06	\$112.48	Q
10-32 UNF to 1/4" Push-to-Connect Tube Fitting	McMaster-Carr	7880T122	8	\$3.31	\$26.48	R
1/4" Push-to-Connect Plug	McMaster-Carr	5779K54	2	\$1.16	\$2.32	S

Table 3: Pneumatic Control System, Module 2: Filter Assembly to House Air

(continued on next page)

Table 3 (continued)

Global requirements by module for full build						
Component	Source	Catalog Number	Quantity	Cost /Unit	Total	Part
3-Way 1/4" Push-to-Connect Manifold	McMaster-Carr	5779K318	2	\$16.60	\$33.20	T
1/4" NPT to 1/4" Brass Push-to-Connect Tube Fitting	McMaster-Carr	7880T125	2	\$2.24	\$4.48	C
Brass Ball Valve, T-handle, 1/4" NPT FxM	McMaster-Carr	4912K92	1	\$7.02	\$7.02	U
Wilkerson Modular Compressed Air Filter, 5 um, 1/4" Connector	McMaster-Carr	60115K19	1	\$70.27	\$70.27	V
Filter Joiner Clamp	McMaster-Carr	60115K22	1	\$13.05	\$13.05	X
Standard Oil vapor and Odor Removal Filter, 0.003 um	McMaster-Carr	7426K11	1	\$80.10	\$80.10	Y
Brass Elbow Fitting, 1/4" NPT, FxM	McMaster-Carr	50785K43	1	\$2.50	\$2.50	E
1/4" Push-to-Connect Plug	McMaster-Carr	5779K54	1	\$1.16	\$1.16	S
Table 4: Pneumatic Control System, Module 3: Control 8-Valve Solenoid Manifolds						
Component	Source	Catalog Number	Quantity	Cost /Unit	Total	Part
4-Way Luer Stopcock, M Lock, F Connectors, Pack of 100	Cole-Parmer	EW-30600-09	0	\$185.00	\$0.00	N
10-32" Special Tapered Thread to Male Luer w 1/4" Hex, Pack of 100	Value Plastics	XMLRL-9	1	\$34.80	\$34.80	a
Finger Snap Luer Lock Ring, Pack of 100	Value Plastics	FSLLR-9002	1	\$14.50	\$14.50	b
Male Luer to Barb Elbow, 1/8" ID Tubing, Pack of 100	Value Plastics	LE7230-9	1	\$50.40	\$50.40	c
Luer Adapter, Pair to Female 1/4"-28	Idex	P-628	48	\$3.90	\$187.20	d
Flangeless Ferrule (ETFE), 1/4"-28 Flat-Bottom, Pack of 25	Idex	P200	2	\$32.75	\$65.50	e
Flangeless Male Nut, 1/4"-28 Flat-Bottom, 1/16" OD Red, Pack of 25	Idex	P202	2	\$32.75	\$65.50	f
1/4" to 5/32" NPTF-M Push-to-Connect	McMaster-Carr	51055K8	48	\$1.99	\$95.52	g
Luer Plug Caps, Pack of 10	McMaster-Carr	51525K311	0	\$2.41	\$0.00	L
Steel Blunt Pins, 1/2" length, Pack of 250	NE Small Tube	NE-1310-02	1	\$212.50	\$212.50	P1
Tee Tube Fitting for 1/8" ID Tubing, Pack of 100	Value Plastics	T230-1	0	\$26.80	\$0.00	K
8-Valve Solenoid Valve Manifold	Festo	MH1A24VDCNH8SVPRK01QMAPBPCXD	6	\$564.71	\$3388.26	h
Table 5: Pneumatic Control System, Module 4: Control Loading						
Component	Source	Catalog Number	Quantity	Cost /Unit	Total	Part
Male Luer Integral Lock Ring, 1/8" barb, Pack of 100	Value Plastics	MTLL230-9	0	\$20.20	\$0.00	M
Female Luer 1/4"-28 Panel Mount to 1/8" Barb, Pack of 100	Value Plastics	FLLB230-1	0	\$19.00	\$0.00	J
Nylon 1/4"-28 Hex Nut, Pack of 100	McMaster-Carr	94812A800	1	\$6.47	\$6.47	i
Scientific Nalgene Polypropelene Wide Mouth Bottle	Cole-Parmer	EW-06057-10	1	\$26.36	\$26.36	j
Luer Lock Manifold, 5 Ports, F Luer, Pack of 10	Cole-Parmer	EW-30600-43	1	\$95.00	\$95.00	k
1-Way Luer Stopcock, M Lock, Pack of 100	Cole-Parmer	Sk-30600-05	0	\$185.00	\$0.00	I
Male Luer Integral Lock Ring, 1/8" barb, Pack of 100	Value Plastics	MTLL430-9002	0	\$20.20	\$0.00	H
Table 6: Digital Modbus Control						
Component	Source	Catalog Number	Quantity	Cost /Unit	Total	Part
WAGO Programmable I/O Controller	WAGO	750-881	1	\$665.00	\$665.00	W1
WAGO AC/DC DIN Rail Power Supply, 240 W	WAGO	787-732	1	\$135.00	\$135.00	W2
WAGO 4-channel digital output, 24 V, 0.5 A	WAGO	750-504	14	\$72.22	\$1011.08	W3
WAGO I/O End Module	WAGO	750-600	1	\$20.00	\$20.00	W5
Mounting Rail, DIN 3 Rail, 35 mm wide, 1 m long	McMaster-Carr	8961K15	1	\$5.07	\$5.07	W6
Ethernet Cable, CAT5E	Digikey	AE10492-ND	1	\$4.66	\$4.66	m
8 ft. Power Cord with SPT-1 NEC Cord	Grainger	1FD95	1	\$7.76	\$7.76	n
Assorted Wire, Red and Black, 18G	Amazon	SW18A08F5C2	1	\$5.98	\$5.98	o
Table 7: Machined Part Cost Estimates						
Baseboard (backboard, laser cut acrylic)	Laser Cut, TAP Plastics		1	\$110.77	\$110.77	-
Flow Control Manifolds (stopcock-mount, 3D printed ABS)	3D Printed, uPrint		6	\$12.00	\$72.00	-
Water Reservoir Stand (reservoir-stand, laser cut acrylic)	Laser Cut, Big Blue Saw		6	\$14.38	\$86.28	-

(continued on next page)

Table 3 (continued)

Global requirements by module for full build						
Control Water Reservoir (reservoir, machined acrylic)	Machined		6	\$105.00	\$630.00	-
OPTION 1 FULL BUILD			TOTAL		\$10,379	

Table 4
WAGO global settings for this implementation.

WAGO Global Setting	File type
WAGO Ethernet Dip Switch	198.168.1.3
Connection Watchdog Timer (Ethernet)	0 (timer off)

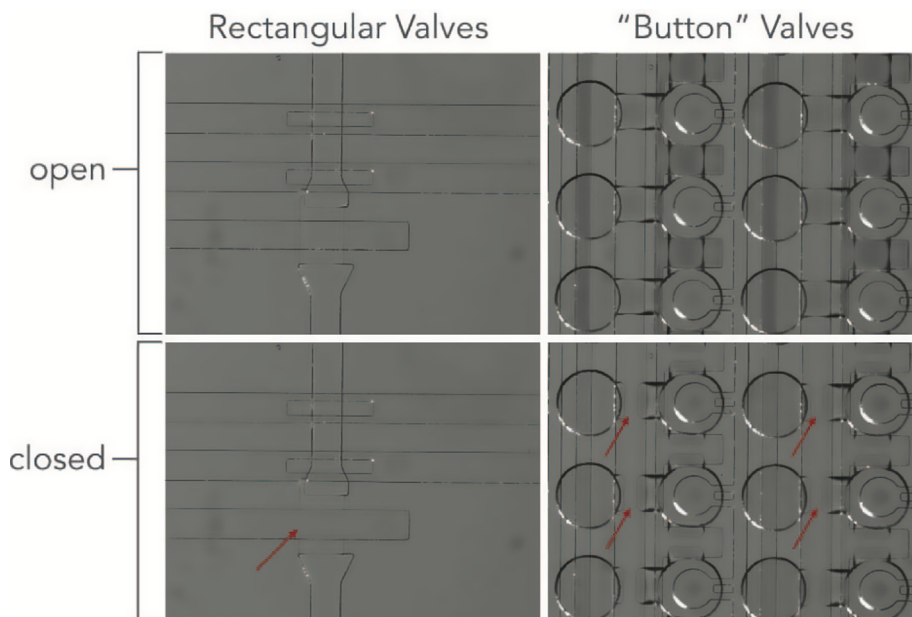


Fig. 11. (a) Valve closed state under 25 psi control on a MITOMI device. (b) Valve open state.

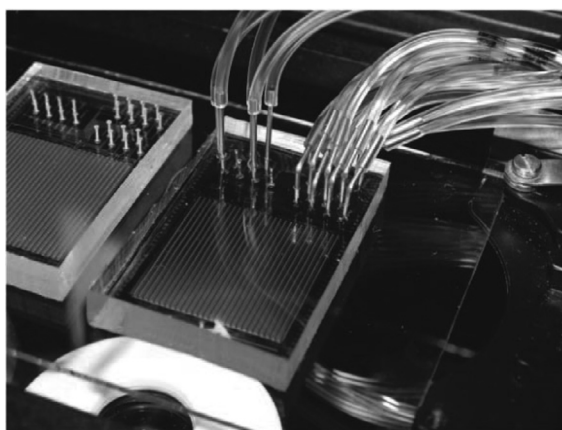


Fig. 12. Image of a fully prepped MITOMI device with control lines and flow lines in operation.

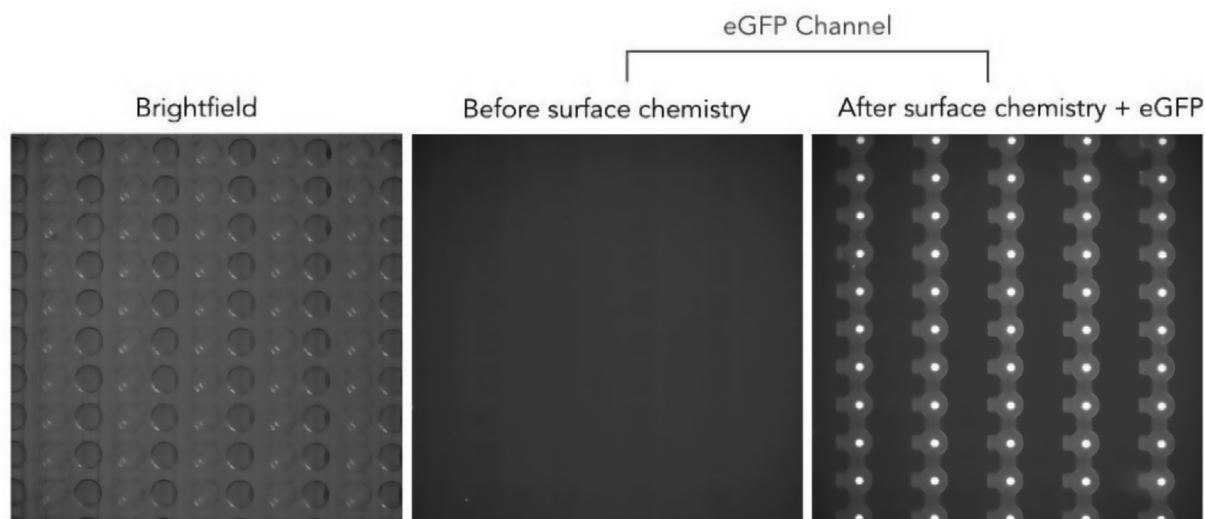


Fig. 13. Experimental results showing an increase in eGFP under only the button area resulting from precise valve-actuation events for successful patterning.

(7) passivate all surfaces *except those beneath the button* by introducing more biotinylated BSA, (8) wash, (9) open button, (10) introduce biotinylated anti-eGFP (which is recruited to neutravidin-coated surfaces beneath the button), and (11) wash. Device preparation and setup for this experiment is described in detail as an example in the **Device Operation Guide.pdf** (Supplement 9).

We then tested if the patterning had been successful by flowing eGFP protein over the device (button valves open) followed by washing and then visualizing the resultant fluorescence in the eGFP channel. Surface patterning and immobilization is shown in Fig. 13, demonstrating that valve actuation and automated control of sample introduction during the experiment were successfully implemented.

9. Discussion

In this report, we provide instructions on how to build a pressure-driven pneumatic setup for universal microfluidic device operation and automated control. This system is capable of driving 18 flow inputs and 48 individually-addressable control line inputs on a microfluidic chip. The setup build is easily adjustable, scalable, and customizable to a user's needs while being cost-effective compared to similar commercial solutions. To demonstrate this modularity, we have presented two additional build options, (1) an abridged programmable setup with fewer control lines and (2) a fully manual setup. With the completion of the build, any user should be able to operate and automate a wide range of microfluidic devices and experiments. This open-source hardware and software build should enable researchers from all fields to take advantage of microfluidic technologies and easily operate their own devices.

Specifications table

Hardware name	An Open-Source, Programmable Pneumatic Setup for Operation and Automated Control of Single- and Multi-Layer Microfluidic DevicesGeppetto (Python-based solenoid valve control software with GUI)Geppetto CLI (Python-based solenoid valve software with command line scripting for experiment automation)
Subject area	<ul style="list-style-type: none"> • Engineering and Material Science • Biological Sciences (e.g. Microbiology and Biochemistry) • General
Hardware type	<ul style="list-style-type: none"> • Biological sample handling and preparation
Open Source License	Pneumatics Instrumentation: GPL 3.0 LicenseGeppetto Software: GPL 3.0 License
Cost of Hardware	Variable, dependent on user customizationFull Build: \$10,380.Abridged Build: \$4455.Manual Build: \$2110.Additional Modification Builds Costs shown in Table 1
Source File Repository	OSF: https://osf.io/jwyau DOI: 10.17605/OSF.IO/JWYAUGithub: github.com/FordyceLab/Open_Source_Pneumatics Supplementary Materials (In Article)

Acknowledgements

The authors acknowledge the Fordyce Lab members, in particular Bianca Cruz, for their helpful comments and feedback on the build revisions and manuscript. This work was supported by NIH/NIGMS Grants R00GM09984804, DP2GM123641, and R01GM107132. P.M.F. acknowledges support from the Beckman Foundation, the Sloan Research Foundation, and a McCormick and

Gabilan faculty fellowship.

P.M.F. is a Chan Zuckerberg Biohub Investigator. K.B. acknowledges support from a TL1 Stanford Clinical and Translational Science Award to Spectrum (NIH TL1 TR 001084) fellowship, a Chemical Biology Interface (CBI) fellowship from the Chem-H Institute (Stanford University) and a NSF GRFP fellowship. C.J. M. acknowledges support from the Canadian Institutes of Health Research (CIHR) postdoctoral fellowship. T.C.S. acknowledges support from a NSF GRFP fellowship. B.C. acknowledges Stanford CAMPARE for support for a summer research rotation at Stanford University.

Appendix A. Supplementary data

Supplementary data associated with this article can be found, in the online version, at <http://dx.doi.org/10.1016/j.ohx.2017.10.001>.

References

- [1] G.M. Whitesides, The origins and the future of microfluidics, *Nature* 442 (2006) 368–373, <http://dx.doi.org/10.1038/nature05058>.
- [2] J. Melin, S.R. Quake, Microfluidic large-scale integration: the evolution of design rules for biological automation, *Annu. Rev. Biophys. Biomol. Struct.* 36 (2007) 213–231, <http://dx.doi.org/10.1146/annurev.biophys.36.040306.132646>.
- [3] D. Mark, S. Haeberle, G. Roth, F. von Stetten, R. Zengerle, Microfluidic lab-on-a-chip platforms: requirements, characteristics and applications, *Chem. Soc. Rev.* 39 (2010) 1153–1182, <http://dx.doi.org/10.1039/b820557b>.
- [4] T.A. Duncombe, A.M. Tentori, A.E. Herr, Microfluidics: reframing biological enquiry, *Nat. Rev. Mol. Cell Biol.* 16 (2015) 554–567, <http://dx.doi.org/10.1038/nrm4041>.
- [5] E.K. Sackmann, A.L. Fulton, D.J. Beebe, The present and future role of microfluidics in biomedical research, *Nature* 507 (2014) 181–189, <http://dx.doi.org/10.1038/nature13118>.
- [6] T.M. Squires, S.R. Quake, Microfluidics: fluid physics at the nanoliter scale, *Rev. Mod. Phys.* 77 (2005) 977–1026, <http://dx.doi.org/10.1103/RevModPhys.77.977>.
- [7] T. Schneider, J. Kreutz, D.T. Chiu, The potential impact of droplet microfluidics in biology, *Anal. Chem.* 85 (2013) 3476–3482, <http://dx.doi.org/10.1021/ac400257c>.
- [8] T.M. Tran, F. Lan, C.S. Thompson, A.R. Abate, From tubes to drops: droplet-based microfluidics for ultrahigh-throughput biology, *J. Phys. D: Appl. Phys.* 46 (2013) 114004–114022, <http://dx.doi.org/10.1088/0022-3727/46/11/114004>.
- [9] M.T. Guo, A. Rotem, J.A. Heyman, D.A. Weitz, Droplet microfluidics for high-throughput biological assays, *Lab. Chip.* 12 (2012) 2146–2155 PB, doi:10.1039/c2lc21147e.
- [10] M.A. Unger, H.-P. Chou, T. Thorsen, A. Scherer, S.R. Quake, Monolithic microfabricated valves and pumps by multilayer soft lithography, *Science* 288 (2000) 113–116, <http://dx.doi.org/10.1126/science.288.5463.113>.
- [11] T. Thorsen, S.J. Maerkl, S.R. Quake, Microfluidic large-scale integration, *Science* 298 (2002) 580–584, <http://dx.doi.org/10.1126/science.1076996>.
- [12] R. Gómez-Sjöberg, A.A. Leyrat, D.M. Pirone, C.S. Chen, S.R. Quake, Versatile, fully automated, microfluidic cell culture system, *Anal. Chem.* 79 (2007) 8557–8563, <http://dx.doi.org/10.1021/ac071311w>.
- [13] Carl L. Hansen, Scott Classen, A. James, M. Berger, Stephen R. Quake, A Microfluidic Device for Kinetic Optimization of Protein Crystallization and In Situ Structure Determination, *Am. Chem. Soc.* 2006. doi:10.1021/ja0576637.
- [14] J. Leng, J.-B. Salmon, Microfluidic crystallization, *Lab. Chip.* 9 (2009) 24–34, <http://dx.doi.org/10.1039/B807653G>.
- [15] C.L. Hansen, E. Skordalakes, J.M. Berger, S.R. Quake, A robust and scalable microfluidic metering method that allows protein crystal growth by free interface diffusion, *Proc. Natl. Acad. Sci. U.S.A.* 99 (2002) 16531–16536, <http://dx.doi.org/10.1073/pnas.262485199>.
- [16] V. Lecault, A.K. White, A. Singhal, C.L. Hansen, Microfluidic single cell analysis: from promise to practice, *Curr. Opin. Chem. Biol.* 16 (2012) 381–390, <http://dx.doi.org/10.1016/j.cbpa.2012.03.022>.
- [17] J.S. Marcus, W.F. Anderson, S.R. Quake, Microfluidic single-cell mRNA isolation and analysis, *Anal. Chem.* 78 (2006) 3084–3089, <http://dx.doi.org/10.1021/ac0519460>.
- [18] Y. Lu, Q. Xue, M.R. Eisele, E.S. Sulistijo, K. Brower, L. Han, et al., Highly multiplexed profiling of single-cell effector functions reveals deep functional heterogeneity in response to pathogenic ligands, *Proc. Natl. Acad. Sci. U.S.A.* 112 (2015) E607–E615, <http://dx.doi.org/10.1073/pnas.1416756112>.
- [19] S.J. Maerkl, S.R. Quake, Experimental determination of the evolvability of a transcription factor, *Proc. Natl. Acad. Sci. U.S.A.* 106 (2009) 18650–18655, <http://dx.doi.org/10.1073/pnas.0907688106>.
- [20] P.M. Fordyce, D. Gerber, D. Tran, J. Zheng, H. Li, J.L. DeRisi, et al., De novo identification and biophysical characterization of transcription-factor binding sites with microfluidic affinity analysis, *Nat. Biotechnol.* 28 (2010) 970–975, <http://dx.doi.org/10.1038/nbt.1675>.
- [21] A.K. White, M. VanInsberghe, O.I. Petriv, M. Hamidi, D. Sikorski, M.A. Marra, et al., High-throughput microfluidic single-cell RT-qPCR, *Proc. Natl. Acad. Sci. U.S.A.* 108 (2011) 13999–14004, <http://dx.doi.org/10.1073/pnas.1019446108>.
- [22] R.E. Gerver, R. Gómez-Sjöberg, B.C. Baxter, K.S. Thorn, P.M. Fordyce, C.A. Diaz-Botia, et al., Programmable microfluidic synthesis of spectrally encoded microspheres, *Lab. Chip.* 12 (2012) 4716–4723, <http://dx.doi.org/10.1039/C2LC40699C>.
- [23] H.Q. Nguyen, K. Brower, B. Harink, B. Baxter, K.S. Thorn, P.M. Fordyce, Peptide library synthesis on spectrally encoded beads for multiplexed protein/peptide bioassays, in: B.L. Gray, H. Becker (Eds.), *SPIE BiOS, SPIE*, 2017: pp. 100610Z–11. doi:10.1117/12.2254908.
- [24] H.Q. Nguyen, B.C. Baxter, K. Brower, C.A. Diaz-Botia, J.L. DeRisi, P.M. Fordyce, et al., Programmable microfluidic synthesis of over one thousand uniquely identifiable spectral codes, *Adv. Opt. Mater.* (2016), <http://dx.doi.org/10.1002/adom.201600548>.
- [25] W.H. Grover, R.H.C. Ivester, E.C. Jensen, R.A. Mathies, Development and multiplexed control of latching pneumatic valves using microfluidic logical structures, *Lab. Chip.* 6 (2006) 623–631, <http://dx.doi.org/10.1039/B518362F>.
- [26] P.M. Fordyce, C.A. Diaz-Botia, J.L. DeRisi, R. Gómez-Sjöberg, Systematic characterization of feature dimensions and closing pressures for microfluidic valves produced via photoresist reflow, *Lab. Chip.* 12 (2012) 4287–4295. doi:10.1039/C2LC40414A.
- [27] D. Marshall, Microfluidics for single cell analysis, *Curr. Opin. Biotechnol.* 23 (2012) 109–118, <http://dx.doi.org/10.1016/j.copbio.2011.11.002>.
- [28] C. Hansen, Microfluidics in structural biology: smaller, faster... better, *Curr. Opin. Struct. Biol.* 13 (2003) 538–544, <http://dx.doi.org/10.1016/j.sbi.2003.09.010>.
- [29] M.L. Kovarik, P.C. Gach, D.M. Ornoff, Y. Wang, Micro total analysis systems for cell biology and biochemical assays, *Analytical ...* (2011).
- [30] D.S. Kong, T.A. Thorsen, J. Babb, S.T. Wick, J.J. Gam, R. Weiss, et al., Open-source, community-driven microfluidics with metafluidics, *Nat. Biotechnol.* 35 (2017) 523–529, <http://dx.doi.org/10.1038/nbt.3873>.
- [31] E.T. da Costa, M.F. Mora, P.A. Willis, C.L. do Lago, H. Jiao, C.D. Garcia, Getting started with open-hardware: development and control of microfluidic devices, *Electrophoresis* 35 (2014) 2370–2377, <http://dx.doi.org/10.1002/elps.201400128>.
- [32] K. Brower, A.K. White, P.M. Fordyce, Multi-step variable height photolithography for valved multilayer microfluidic devices, *JoVE* (2017) 1–12. doi:10.3791/55276.
- [33] R. Gómez-Sjöberg, Rafael's Microfluidics Site, (n.d.). Available from: <https://sites.google.com/site/rafaelsmicrofluidicspage/valve-controllers>.
- [34] A.K. White, K.A. Heyries, C. Doolin, M. VanInsberghe, C.L. Hansen, High-throughput microfluidic single-cell digital polymerase chain reaction, *Anal. Chem.* 85 (2013) 7182–7190, <http://dx.doi.org/10.1021/ac400896j>.
- [35] S.J. Maerkl, S.R. Quake, A systems approach to measuring the binding energy landscapes of transcription factors, *Science* 315 (2007) 233–237, <http://dx.doi.org/10.1126/science.1131007>.
- [36] D.I. Walsh III, D.S. Kong, S.K. Murthy, P.A. Carr, Enabling microfluidics: from clean rooms to makerspaces, *Trends Biotechnol.* 35 (2017) 383–392, <http://dx.doi.org/10.1016/j.tibtech.2017.01.001>.